

OPENLAB VERIFIED · Report identity and source-transcribed quantity. Compound purity and analytical events retain their separate source scopes.

TRENAVAR

Lab record

Batch	Laboratory	Report	Analysed
OL2207	Janoshik Analytical	28940	18 April 2023

Powered by EvidenceOS, connecting this Olympus Labs UK product and batch to its laboratory results and source evidence.

Trenavar · Concentration

27.03 mg

Reported sample; the laboratory gives mg without a per-capsule denominator.

Janoshik report 28940 · OL2207

Trenavar · Purity

97.48%

Compound raw material

Olympus Labs UK · compound purity statement

REPORTED

Compound identity

Trendione

REPORTED

Reported quantity

27.03 mg

REPORTED

Compound purity

97.48%

REPORTED

Laboratory source

Janoshik

REPORTED

Batch connection

OL2207

REPORTED

Sample receipt

2023-04-14

The batch report and supporting compound analyses retain their separate dates and source identities. Compound raw-material purity is a supporting observation; production stage is unspecified.



Compound analysis

Trendione · LC/MS chromatogram · 2022-08-16

LC/MS 16 August 2022 DAD1 B, 220 nm

LC/MS Report

File D:\CHEM32\DATA\202208\20220816-KEHU-1 2022-08-16 16-58-11\4911-20220816-LCMS.D
Injection Date : 16-Aug-22, 17:26:23 Tgt Mass (EZ) :
Sample Name : Location : P1-F-03
Acq. Operator : Inj : 1
Spec. Reported : MS Integration Inj Volume : 3 ul
Acq. Method : D:\CHEM32\DATA\202208\20220816-KEHU-1 2022-08-16 16-58-11\401-CZ-RK.M
Analysis Method : C:\Chem32\1\METHODS\401-GP50-KEHU.M
Sample Info :
Method Info : Instrument : Agilent 1200-6110 MS
Mobile Phase : A=0.1%TFA in water, B=Acetonitrile
Gradient : 5-95% B in 4 min, 95%B in isocratic for 3min
Flow Rate : 0.6 mL/min
Column : XDB-C18 2.1*50mm, 3.5um
Column temperature : 35°C

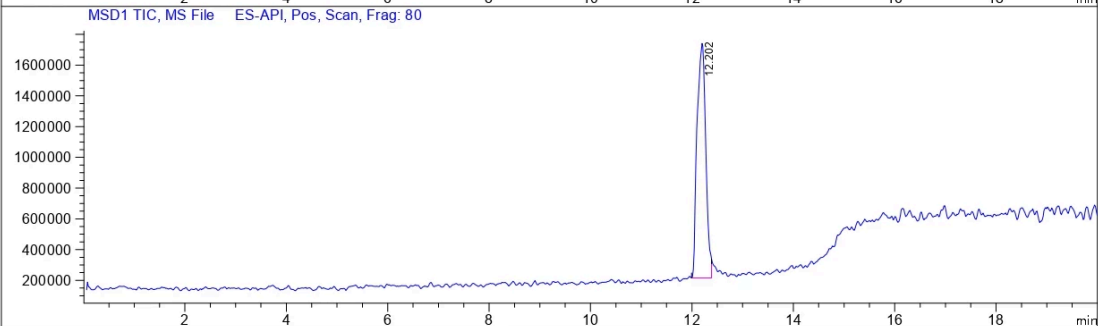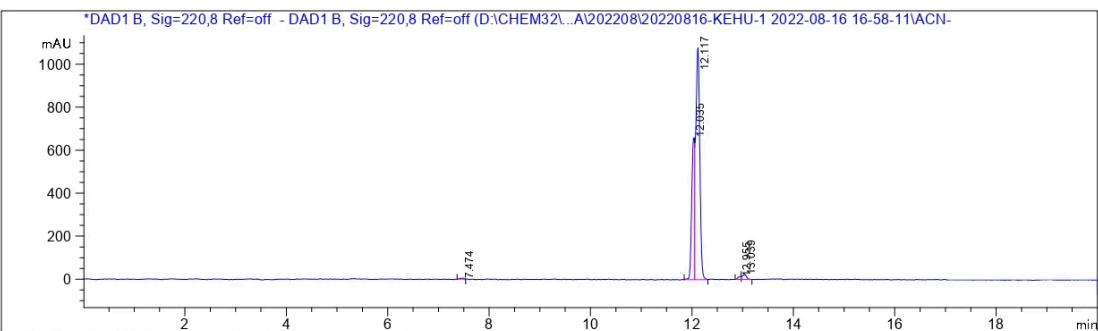

Integration Results for DAD1 B, Sig=220,8 Ref=off

RetTim	Width	Area	Height	Area%
7.47	0.08	26.42	4.86	0.30
12.03	0.06	2578.15	661.52	29.39
12.12	0.08	5972.22	1079.62	68.09
12.96	0.07	59.72	14.21	0.68
13.04	0.08	134.33	22.83	1.53

Compound analysis


Trendione · mass spectrum · 2022-08-16

LC/MS 16 August 2022 Original source spectrum

LC/MS Report

Ret. Time: 12.20

<<<< POSITIVE SPECTRA >>>>

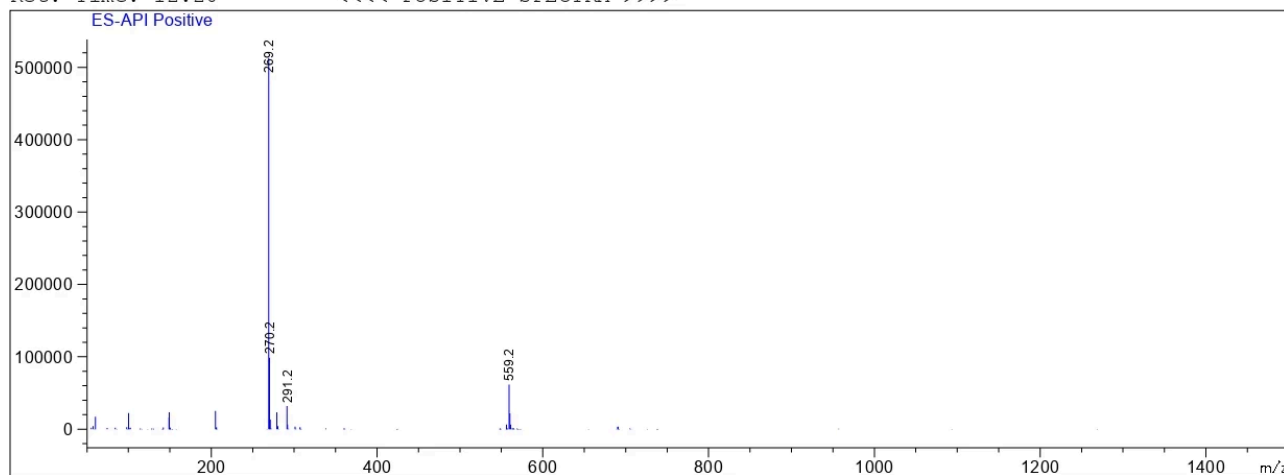

Original analytical page · Supporting compound evidence

Sample analysis

TRENAVAR · PDA Ch1 220–260 nm · 2023-04-14

Chromatography 14 April 2023 PDA Ch1 220–260 nm




Analysis Report

<Sample Information>

Sample Name : 1275-3
Method Filename : Raws - blind common anabolic steroid and aromatase inhibitors screening.lcm
Vial # : 3-3
Injection Volume : 0.5 uL
Date Acquired : 14/04/2023 10:36:03
Date Processed : 14/04/2023 10:40:37
Sample Type : Unknown
Acquired by : Janoshik s.r.o.
Processed by : Janoshik s.r.o.

<Chromatogram>

mAU

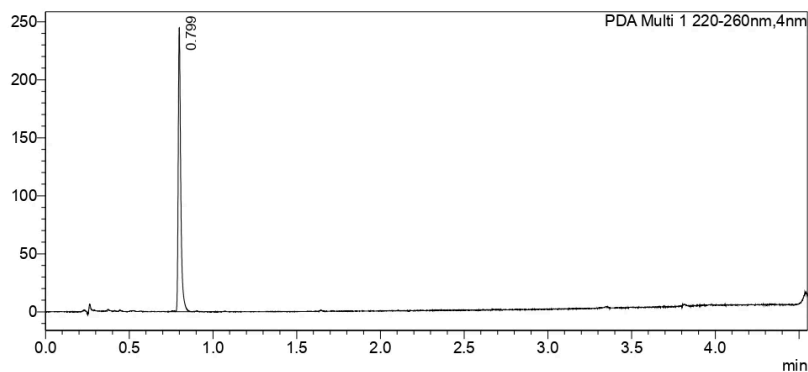

<Peak Table>

PDA Ch1 220-260nm

Peak#	Ret. Time	Area	Name
1	0.799	254213	
Total			

info@janoshik.com

Original analytical page · Report 28940

Sources and record edition

TEST REPORT



E-mail: info@janoshik.com
Web: www.janoshik.com

Task Number

#28940

Testing ordered >

31 MAR '23

Sample received >

14 APR '23

Client

support@olympuslabs.uk

Sample

TRENAVAR 30MG

Manufacturer

Olympus Labs UK

Batch

OL2207

Sample description >

Pictures not included.

Tests requested >

Qualitative and quantitative analysis of non-AAS sample.

Results >



Trendione	27.03 mg

Comments >

Analysis conducted >

18 APR 2023

Signature >



Verify this test at www.janoshik.com/verify/ with the following unique key

5YGFY9QGWPJC

Laboratory dates

Sample received: 14 April 2023

Analysed: 18 April 2023

Janoshik · 28940

[View source](#)

598c83d1d48d2e591d59a4f7a14622e83e41418527d402ec18ef2d1f8399bd24

Trendione · LC/MS chromatogram · 2022-08-16

Source image included in this edition.

59f7ba4304412756bd385fcb36c3168c927aae406249ac718ff829e18deea5c2

Trendione · mass spectrum · 2022-08-16

Source image included in this edition.

4c8fdb7aa0be5c061a9f12c1bf00355430a55cbc2c3e0fddeb518346a9284a9b

Janoshik report 28940

[View source](#)

af882ca6959c2416abe6f6f63de1c496fc018b9452a23d1ecc32953ee4595247

TRENAVAR · publisher purity statement

[View source](#)

f3d748be0be39c543c094d37a73cf004a78a7e90cc1812198534611fb8fdce4f

TRENAVAR · PDA Ch1 220-260 nm · 2023-04-14

[View source](#)

cc505eedd60baa428a8130c2d81f996c152a3bc2edb32cb817edfacee46b3315

Edition

openlab.v2.a96fcafd660adcc3

Record digest:

6242822e30a56d1cd98aaa27b979c9b0c1dc0861a90066a4b5fb48a502aff1de